


ICP® & CHARGE FORCE SENSORS


Theory of Operation

Piezoelectric force sensors measure compressive or tensile loads for a wide variety of applications. They incorporate a piezoelectric sensing element with a crystalline atomic structure which outputs an electrical charge when subjected to force with near zero deflection. The charge output occurs instantaneously, making piezoelectrics ideal for dynamic applications but subject to decay and therefore not capable of static measurements.

PCB® force sensors are constructed with thin quartz crystal discs as the piezoelectric sensing elements which are "sandwiched" between upper and lower base plates. The base plates are compressively loaded together to a specific preload setting and retained by either a preload stud (threaded) or pre-load sleeve (welded). The sensing elements are preloaded, allowing for tensile measurements. Electrodes on the sensing elements transfer the electrical charge to internal ICP® electronics or directly to the electrical connector in charge models. The outer housing aligns internal components, provides structural support for the electrical connector, and is hermetically welded to the base plates for ingress protection. This compressively loaded stack results in extraordinary stiffness for precision measurement under dynamically cycling loads.



Typical PCB® Force Sensor



Two Main Types of Piezoelectric Force Sensors

- ICP® - Identifies PCB sensors that incorporate built-in microelectronics. The ICP® electronics convert a high-impedance charge signal generated by a piezoelectric sensing element into a usable low-impedance voltage signal when powered with constant current. The modified signal can be readily transmitted over two-wire or coaxial cables to data acquisition systems or readout devices.
- Charge Mode - The output of a charge mode force sensor is a high impedance signal which is dependent on electrical insulation for low loss / low noise transmission. It should be converted to a low impedance signal prior to the data acquisition system or readout device. It is important to use low noise cables and avoid using cables with insulation damage or contamination.

ICP® Advantages

- Simple to operate
- Able to operate in dirty environments over long cable runs
- Uses integral power from all manufacturers' data acquisition systems (may require specific module)

Disadvantages

- Maximum operating temperature of 250 °F (121 °C)
- Sensitivity and low frequency response are not adjustable
- Requires ICP® constant-current power

Charge Mode Advantages

- Operating temperature up to 400 °F (204 °C)
- Flexibility in adjusting output characteristics
- Extended low frequency response with long time constant charge amps

Disadvantages

- Additional cost of required charge amplifier or charge converter
- Sensor and cable connections must be kept clean and dry for best performance
- Requires more costly, low noise cable

Amplitude Range of PCB Force Sensors

Most ICP® force sensors have a full scale output voltage of 5 volts. Charge force sensors are not limited to a maximum 5 volt full scale output range, they can operate anywhere within the linear measurement range listed on the specification sheet. The charge output (pC/lb force) can then be converted by a charge amplifier or charge converter (mV/pC). Laboratory amplifiers typically have the ability to adjust gain and measurement range. In-line charge converters typically have a fixed gain and measurement range.

ICP® Measurement Output

Force Sensitivity (FS): 500 mV/lb  
Measurement Range (MR): 10 lb compression  
Signal Output (V<sub>o</sub>) = FS x MR  
= 500 mV/lb x 10 lb  
V<sub>o</sub> = 5,000 mV = 5.0 volts

Charge Measurement Range

The max force measurable with this sensor and converter combination  
Force Sensitivity (FS): 18 pC/lb  
Converter Input Range (CI): ± 5,000 pC  
Measureable Force (MF<sub>max</sub>) = CI + FS  
= ± 5,000 pC + 18 pC/lb  
MF<sub>max</sub> = ± 277.8 lb  
(Necessary preload must be considered for tension)

Charge Gain Conversion

Force Sensitivity (FS): 18 pC/lb  
Force Input (F<sub>i</sub>): 75 lb  
Charge Conversion (CC): 1 mV/pC  
Signal Output (V<sub>o</sub>) = FS x F<sub>i</sub> x CC  
= 18 pC/lb x 75 lb x 1.0 mV/pC  
V<sub>o</sub> = 1,350 mV = 1.4 volts

Conversion Units


1 lb (pound force) = 4.45 N (newton)  
1,000 lb = 4500 N = 4.45 kN

ELECTRONICS FOR ICP® & CHARGE FORCE SENSORS

ICP® Force Sensor Instrumentation

ICP® force sensors must be powered from a constant-current DC voltage source (see specific sensor datasheet for turn-on voltage). Once powered, the electronics within an ICP® sensor convert piezoelectric charge to a low impedance signal with power and output on the same channel. ICP® signal conditioners or ICP® configured readout devices will remove the power portion of the signal, resulting in full scale output of ± 5 volts.

PCB offers multiple ICP® signal conditioners from 1 to 16 channels with current adjustment within 2 - 20 mA at +18 to +30 volts DC. Refer to PCB Tech Note TN-32 for more information on signal conditioners and impedance. Do not attempt to power ICP® sensors with commercially available power supplies as unregulated current will damage the sensors' internal electronics.





When a data acquisition system (DAQ) includes ICP® power, a separate signal conditioner is not required.



Charge Force Sensor Instrumentation

Charge mode sensors' high impedance signal requires conversion to a low impedance voltage signal prior to being processed by data acquisition or readout devices. The conversion can be done in two ways:




STRAIN SENSORS

Strain gages vs dynamic strain sensors with ICP®

Traditional strain measurement relies upon resistive strain gages bonded to the surface of the object under test in a 4-element strain gage bridge resulting in the Wheatstone Bridge Circuit. Wheatstone Bridges for strain are commonly used for static measurements and are common to load cells. Although traditional strain gages are low cost, they require suitable adhesive for bonding, have limited dynamic use up to 12 kHz, and are destroyed if removed.

PCB has combined piezoelectric crystals and ICP® technologies for use in dynamic strain measurement. The resulting sensors measure high frequency changes in strain with exceptional linearity over their measurement range. Sensitivity is specified for each sensor in millivolts per microstrain (mV/µε) with full scale output of 5.0 volts. These sensors have two mounting options: to be adhesive bonded to the dynamically loaded structure or mounted with a single through-bolt. The through-bolt design relies upon mechanical friction of contact pads and senses the change in strain between the pads.

Typical Wheatstone Bridge for static strain gage




740B02 Applications:


- Localized wing deflection
- Composite pressure vessel fatigue analysis
- Active vibration control
- Noise path and modal transfer path analysis

RHM240 Series Applications:

- Developed to indirectly measure repetitive impulse loading of machinery structures such as in press force/crimping or tooling fatigue tracking.
- Machine Frame Deflection - during pressing, crimping, welding for quality control
- Machine press overload protection
- Active vibration control
- Monitor manufacturing process repeatability
- Detection of installed stress on critical equipment



Model 740B02 strain sensors installed on a composite wing structure.




The RHM240 series strain sensor monitors press-force forces to ensure quality end products.

FORCE SENSOR INSTALLATION

Mounting Precision

PCB force sensors are precisely machined and assembled during the production process to maximize uniform transfer of force through the load bearing surfaces of the sensor. Force sensor assemblies require precise alignment of the sensor and contact surfaces to eliminate potential causes for test error. Proper mounting of PCB force rings includes:

- Prepare Mating Surfaces - flat and parallel to within 0.001 in (0.03 mm) total indicated runout and free of any debris. Finish surfaces should be ground smooth to at least 125 microns (3.2 micrometers).
- Monitor Fastener Torque - Excessive fastener torque during assembly and preload can transfer shear load into the force ring and potentially damage the sensor. Observe the following precautions, including those in the specific sensor product manual:
  - Utilize anti-friction washers and fasteners with alignment bushings.
  - Apply a thin layer of lubricant on mounting surfaces during installation (creates better contact between the sensor and mounting surface).
- Careful handling - shock loads from metal to metal impact can damage quartz elements.
- Consider assembly materials and related impact / damping potential.




Force Transfer

- Minimize side / edge loading or bending moments in assemblies.
- Position sensors with axial loading only.
- Tension measurements require proper preloading (see force link assemblies - factory preloaded).
- Preloading a sensor off alignment can mechanically deform the sensor and crack the sensing element internally - output could be reduced or zero, factory evaluation or replacement may be required.

AC Coupled Output vs. DC Coupled Output

The following graph details a cyclical impulse in both AC and DC coupled modes, highlighting the DC offset that is removed by the signal conditioner. Note the low frequency content within only the DC Coupled signal after FFT to Frequency Domain (Amplitude vs Frequency). This is lost in AC Coupled mode.



Long Duration Events and DTC

It is often desired to measure an input pulse lasting a few seconds in duration. This is especially true with force sensor applications where static calibration or quasi-static measurements take place. Before performing tests of this nature, it is important to DC couple the entire monitoring system (signal conditioner and data acquisition) to prevent rapid signal loss.

The general rule of thumb for such measurements is that the output signal loss and time elapsed over the first 10% of a DTC have a one to one relationship. If a sensor has a 500 second DTC, over the first 50 seconds, 10% of the original input signal will have decayed. For 1% accuracy, data should be taken in the first 5% of the DTC. If 9% accuracy is acceptable, the measurement should be taken within 8% of the DTC, and so forth.


Left unchanged, the signal will naturally decay toward zero. This will take approximately 5 times the DTC.

FREQUENCY RESPONSE & RANGE OF ICP® & CHARGE FORCE SENSORS

Discharge Time Constant

- Discharge Time Constant (DTC) is the time (usually in seconds) required for an AC coupled device or measuring system to discharge its signal to 37% of the original value from a step change of measurement.
- Follows RC circuit principles where an instantaneous charge immediately begins dissipating at an exponential rate.
- ICP® sensors have fixed DTC based on the values of the internal RC network. When used in AC coupled systems, (sensor, cable, and ICP® signal conditioner) the sensor will take on the DTC characteristics of the ICP® sensor or signal conditioner (whichever is shortest). In charge mode sensors, the DTC is dictated by choice of charge amplifier or in-line charge converter and system resistance/capacitance.

The graphic below shows the relationship between sensitivity and frequency:



Where: q = instantaneous charge (pC)  
Q = initial quantity of charge (pC)  
R = bias (or feedback) resistor value (ohms)  
C = total (or feedback) capacitance (pF)  
t = any time after t<sub>0</sub> (sec)  
e = base of natural log (2.718)

Low Frequency Response

In ICP® sensors, the low frequency response is dictated by the sensor electronics. Charge mode sensors do not include low frequency response or DTC in their specifications because they are dependent on the specific charge converter or amplifier used. When using charge mode sensors, refer to the specifications of the specific signal converter for low frequency and time constant information.

ICP® sensors have internal microelectronics that perform the conversion from a high impedance charge to a low impedance voltage signal. The low frequency roll off characteristics are included on ICP® sensor datasheets. Example specifications are included in the table below.

Resonant Frequency

At the component level, force sensors capabilities follow a similar curve to that shown above with a resonant frequency limit but they tend to take on the characteristics of the systems they are installed with. Their frequency response tends to be dependent on the stiffness of the overall system, related preloading, and coupling dynamics. Characterization of the installed system is often recommended to determine the frequency measurement threshold. Force test fixtures commonly exhibit natural frequencies in the 2,000 to 4,000 Hz and it is rare to use force sensors beyond these limits.

Typical Performance Specifications

ICP® Force Ring	Model 205C	Charge Force Ring	Model 215B
Sensitivity	0.08 mV/lb	18 pC/lb	4,047 pC/kN
Measurement Range (Comp)	≤ 60,000 lb	≤ 60,000 lb	≤ 266.9 kN
Max Static Force (Compression)	≤ 70,000 lb	≤ 70,000 lb	≤ 311.4 kN
Low Frequency Response	0.0003 Hz, calculated from discharge time constant.	Low frequency response is determined by external signal conditioning electronics.	
Upper Frequency Limit	50,000 Hz	Upper Frequency Limit	50,000 Hz
Non-Linearity	≤ 1.5 % Full Scale	Non-Linearity	≤ 1.5 % Full Scale
Environmental		Environmental	
Temperature Range (Operating)	-65 to +250 °F	Temperature Range (Operating)	-100 to +400 °F
Electrical		Electrical	
Discharge Time Constant	≥ 2,000 sec at room temperature	Capacitance (Typical)	38 pF
Constant Current Excitation	2 to 20 mA	Insulation Resistance	≥ 1.0 E <sup>11</sup> ohms
Output Polarity	Positive in Compression	Output Polarity	Negative in Compression
Physical		Physical	
Preload	12,000 lb	Preload	12,000 lb
Stiffness	40 lb/µin	Stiffness	40 lb/µin


Effect of Excitation Voltage on the Dynamic Range of ICP® Sensors

The specified excitation voltage for all standard ICP® sensors and amplifiers is generally within the range of +18 to +30 volts. The effect of this range is shown in the chart at right.

To explain the chart, the following values will be assumed:

- V<sub>B</sub> = Sensor Bias Voltage = 10 volts
- V<sub>1</sub> = Supply Voltage 1 = 24 volts
- V<sub>2</sub> = Excitation Voltage 1 = V<sub>1</sub> - 1 = 23 volts
- V<sub>3</sub> = Supply Voltage 2 = 18 volts
- V<sub>4</sub> = Excitation Voltage 2 = V<sub>3</sub> - 1 = 17 volts


Note that an approximate 1 volt drop across the current limiting diode (or equivalent circuit) must be maintained for correct current regulation.

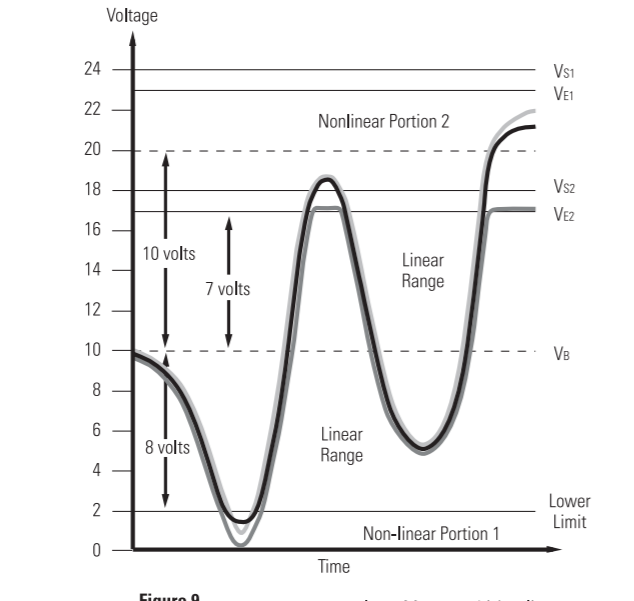


Combining Multiple Force Sensors into Arrays:

Complex force arrays typically involve summation of forces (and moments if triaxial sensors are used). There are two methods to do this when using PCB piezoelectric force sensors:

- Post-data acquisition, (most common) mathematically sum forces and moments about center using derived calculations such as shown below to account for sensor distance from centerline.
- Signal Summing, sum forces and moments about center using derived calculations such as shown below to account for sensor distance from centerline.



Three Axis ICP® Force Plate (note all axes are aligned)



**Axial Forces:**  
 $F_x = [ F_{x1} + F_{x2} + F_{x3} + F_{x4} ]$   
 $F_y = [ F_{y1} + F_{y2} + F_{y3} + F_{y4} ]$   
 $F_z = [ F_{z1} + F_{z2} + F_{z3} + F_{z4} ]$

**Moments about Center:**  
 $M_x = b^* [ F_{z1} + F_{z2} - F_{z3} - F_{z4} ]$   
 $M_y = a^* [ -F_{x1} + F_{x2} + F_{x3} - F_{x4} ]$   
 $M_z = b^* [ (F_{x1} + F_{x4}) - (F_{x2} + F_{x3}) ]$   
 $+ a^* [ (F_{y1} + F_{y4}) - (F_{y2} + F_{y3}) ]$