


Cascade Technical Sciences, Inc.

Reports

IP55 Rated for Protection Against Ingress of Water,
Report CTC1975-1

IP55 Rated for Protection Against Dust,
Report CTC1975-2

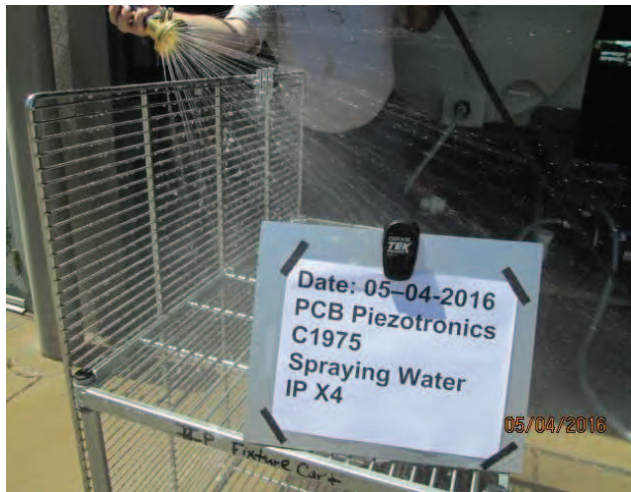

PCB Piezotronics Model 130A24

Water and Dust Resistant Microphone and Preamplifier



Cascade Technical Sciences, Inc.
Hillsboro, Oregon/Longmont Colorado

Report CTC C1975-1

May 19, 2016

For: PCB Piezotronics

Prepared By: Meg Talbert Digitally signed by Meg Talbert
DN: cn=Meg Talbert, o=Element Materials Technology, ou=Quality
email=Meg.Talbert@element.com, c=US
Date: 2016.05.19 23:31:10 -0600'

 Element Denver Quality Administrator 05/19/2016
Date

Reviewed By: Joe Fratiello Digitally signed by Joe Fratiello
DN: cn=Joe Fratiello, o=Element Materials
Technology, ou=Laboratory,
email=Joe.Fratiello@Element.com, c=US
Date: 2016.05.24 12:59:45 -0600'

 Element Denver Laboratory Manager 05/20/2016
Date

Concurred With: Joe Fratiello Digitally signed by Joe Fratiello
DN: cn=Joe Fratiello, o=Element Materials
Technology, ou=Laboratory,
email=Joe.Fratiello@Element.com, c=US
Date: 2016.05.24 16:08:57 -0600'

 Element Portland Quality Manager 05/20/2016
 (Denver Lab Manager signing in absence of QM) **Date**

EAR Controlled Data: This document contains technical data whose export and re-export/retransfer is subject to control by the U.S. Department of Commerce under the Export Administration Act and the Export Administration Regulations. The Department of Commerce's prior written approval may be required for the export or re-export/retransfer of such technical data to any foreign person, foreign entity or foreign organization whether in the United States or abroad.

These commodities, Technology, or software were exported from the United States in accordance with the Export Administration Regulations. Diversion contrary to U.S. law is prohibited.

It is our policy to retain components and sample remnants for a minimum of 30 days from the report date, after which time they may be discarded. The data herein represents only the item(s) tested. This report shall not be reproduced, except in full, without prior permission of Cascade Technical Sciences.

This project shall be governed exclusively by the General Terms and Conditions of Sale and Performance of Testing Services by Cascade Technical Sciences. In no event shall Cascade Technical Sciences be liable for any consequential, special or indirect loss or any damages above the cost of the work.

Administrative Data

Prepared for: PCB Piezotronics
3425 Walden Ave
Depew, NY 14043

Test Facility: Cascade Technical Sciences, Inc.
1530 Vista View Drive
Longmont, CO 80504

Test(s) Performed	Test Specification (Paragraph/Section)
Spraying Water (IP-X4)	CEI/IEC 60529:2013 Para. 14.2.4
Jet Spray (IP-X5)	CEI/IEC 60529:2013 Para. 14.2.5

Item(s) Tested (Description)	Part Number(s)	Serial Number(s)
Microphones	130A24	44296
Microphones	130A24	44293
Microphones	130A24	44292

Rev.	Reason For Revision	Date	Approval
---	Report Issued.	05/19/2016	MJT

Date Test Items Received: 03/01/2016

Testing Initiated Date: 05/04/2016

Testing Completed Date: 05/04/2016



Cascade Tek – Hillsboro, Oregon/Longmont, Colorado

May 19, 2016

Certification No: CTC C1975-1

Attention: Mr. Michael Thibeault
PCB Piezotronics
3425 Walden Ave
Depew, NY 14043

Reference: a. CTek Job No.: C1975
b. CTek Quote No.: 18127A
c. Customer Purchase Order No.: WE00005021
d. Technical Specification: 1. CEI/IEC 60529: 2013

Cascade Technical Sciences, Inc. hereby certifies that the following test sample(s) were subjected to the following test(s).

Quantity	Description	Model/Part Number	Serial Number(s)
1	Microphones	130A24	44296
1	Microphones	130A24	44293
1	Microphones	130A24	44292

1. Spraying Water (IP-X4) Test per Reference (b) Item 1 and (d1), the non-operating samples were subjected to 5 minutes of spraying water exposure at 180 degrees from vertical, using a nozzle per Fig. 5 (reference d1), and a flow rate of ten liters/minute. No visible water ingress was observed.
2. Jet Spray (IP-X5) Test per Reference (b) Item 2 and (d1), the non-operating samples were subjected to 3 minutes of water jet spray exposure, from a distance of 2.5 – 3 meters, using a nozzle per Fig. 6 (reference d1), with a 6.3 mm internal diameter, and a delivery rate of 12.5 liters/minute. No visible water ingress was observed.

Testing was done in accordance with the above references as evidenced and reported in the accompanying data. The test samples were returned to the customer for evaluation.

The original of this report is on file at Cascade Technical Sciences, Inc. under the above referenced certification number for review by authorized personnel. The results of the testing reported herein relate only to the actual items tested.

Respectfully submitted,



Meg Talbert

Quality Administrator

Cascade Technical Sciences, Inc.

This test certification shall not be reproduced, except in full, without written authorization from Cascade Technical Sciences, Inc.

The objective of this test program was to subject customer provided test hardware to environmental simulation in compliance with customer stated specification, including any authorized modification, deviations or concessions to the original requirements. The hardware consisted of items identified in the appropriate sections of this report. In addition to test hardware identification, each section contains information that describes the associated test setup and performance and the resulting data. Cascade Technical Sciences, Inc. measuring instruments used in testing were calibrated according to the requirements of ANSI/NCSL Z540-1 and ISO/IEC 17025, and are traceable NIST or NMI. Calibration records are on file and available for inspection by request. Because the test methods are well established and are qualitative or semi-quantitative in nature, Cascade Technical Sciences, Inc., Inc. does not apply measurement uncertainty unless obligated by contract. Any test hardware operational setups and resulting evaluations or inspections performed by the customer are not included in this report, unless they were explicitly requested. While observations and/or specification compliance statements may be reported, no interpretations or opinions regarding customer product performance are intended. Unless otherwise indicated in the appropriate report section, all contract obligations were met and the test objective achieved.



Test Data Log – Protection Against Water (IPX1 through IPX9)

Section 1 – Customer and Test Information

Job Number: C1975

Customer: PCB Piezotronics

Date Started: 5/4/2016

Date Completed: 5/4/2016

QA Reviewer: Meg Talbert

Signature: *Meg Talbert*

Responsible Technician: Keefe Hart

Quote Issued By: Joe Fratiello

Customer Witness: No Yes Name: N/A

Section 2 – Test parameters

Type of Test: Protection Against Water Intrusion

Test Specification: IEC 60529:2013 Ed. 2.2, Sec. 14.2.4

Test Description:

- IP Designation: IPX4
- Test Means: Spray nozzle ± 180° from vertical.
- Water Flow Rate: 10 l/min ±5 %
- Water Temperature: The water temperature does not differ from that of the specimen by more than 5° K.
- Water Pressure: N/A
- Instructions on Disassembling the Specimen Have Been Received: Yes No
- Passing Criteria: In general, if any water has entered, it shall not:
 - Be sufficient to interfere with the correct operation of the equipment or impair safety.
 - Deposit on insulation parts where it could lead to tracking along the creepage distances.
 - Reach live parts or windings not designed to operate when wet.
 - Accumulate near the cable end or enter the cable if any.
- Additional Instructions: Spraying Water: Samples to be sprayed 180 degrees from vertical using a nozzle per Figure 5. Water flow shall be at a rate of 10 L/min for a period of 1 minute per square meter of enclosure for a minimum of 5 minutes. Water temperature shall not differ by more than 5K from sample temperature.

Section 3 – Test Sample Information

Sample Description	Sample P/N or Model No.	Sample S/N or Other Identifier	Qty.
Microphones	130A24	44296	1
Microphones	130A24	44293	1
Microphones	130A24	44292	1

Section 4 – Test Equipment

ID No.	Description	Manufacturer	Model No.	Serial No.	Last Cal	Next Cal
FR429	Spray Nozzle	Guangzhou Zhilitong Electromechanical	ZLT-JL1	JL011305	06/24/15	06/24/16
FR506	Stop Watch	Digi-Sense	94460-28	160157786	01/28/16	01/28/18
FR66	Tape Measure	Stanley	LeverLock	30-824	Verified Before Use	
FR135	Thermometer	Fluke	54 II B	20380005	06/17/15	06/17/16
FR512	Temperature/ Relative Humidity Meter	Cole-Parmer	90080-03	160173042	03/05/16	03/05/18

Section 5 – Test Log

Customer Name: PCB Piezotronics
 Job Number: C1975

Laboratory Temperature: +71°F
 Laboratory Humidity: 26% RH

Initials	Date	Time	Notes	Photo
KH	5/4/2016	1100	Samples are mounted in a vertical orientation. The exposure will concentrate on the microphone end of the sample opposite the cable end. This is per customer instruction.	<input checked="" type="checkbox"/>
KH	5/4/2016	1120	Water temperature is +16.2°C and sample temperature is +20.2°C; no thermal conditioning is necessary.	<input type="checkbox"/>
KH	5/4/2016	1145	Spray nozzle calibration is verified.	<input type="checkbox"/>
KH	5/4/2016	1155	Begin the 5 minute exposure.	<input checked="" type="checkbox"/>
KH	5/4/2016	1200	Exposure is complete.	<input type="checkbox"/>
KH	5/4/2016	1205	Remove the samples from the spray cart and hand dry the exterior of the sample.	<input type="checkbox"/>
KH	5/4/2016	1210	Unscrew the cover on the microphone end and dry the interior surface exposed under the cover.	<input type="checkbox"/>
KH	5/4/2016	1210	Peel back the adhesive membrane material and inspect for any indication of water ingress.	<input type="checkbox"/>
KH	5/4/2016	1215	There is no sign of water below the peel back membrane. Install new membrane pads on each sample for subsequent testing.	<input checked="" type="checkbox"/>
KH	5/4/2016	1230	Samples will progress on to IPX5 level spray test.	<input type="checkbox"/>
KH	5/4/2016	1245	IPX4 testing is complete.	<input type="checkbox"/>

CASCADE
TEK
WITH EXPLORER

Date: 05-04-2016
PCB Piezotronics
C1975
Spraying Water
IP X4

05/04/2016




Date: 05-04-2016
PCB Piezotronics
C1975
Spraying Water
IP X4

05/04/2016



Date: 05-04-2016
PCB Piezotronics
C1975
Spraying Water
IP X4

05/04/2016

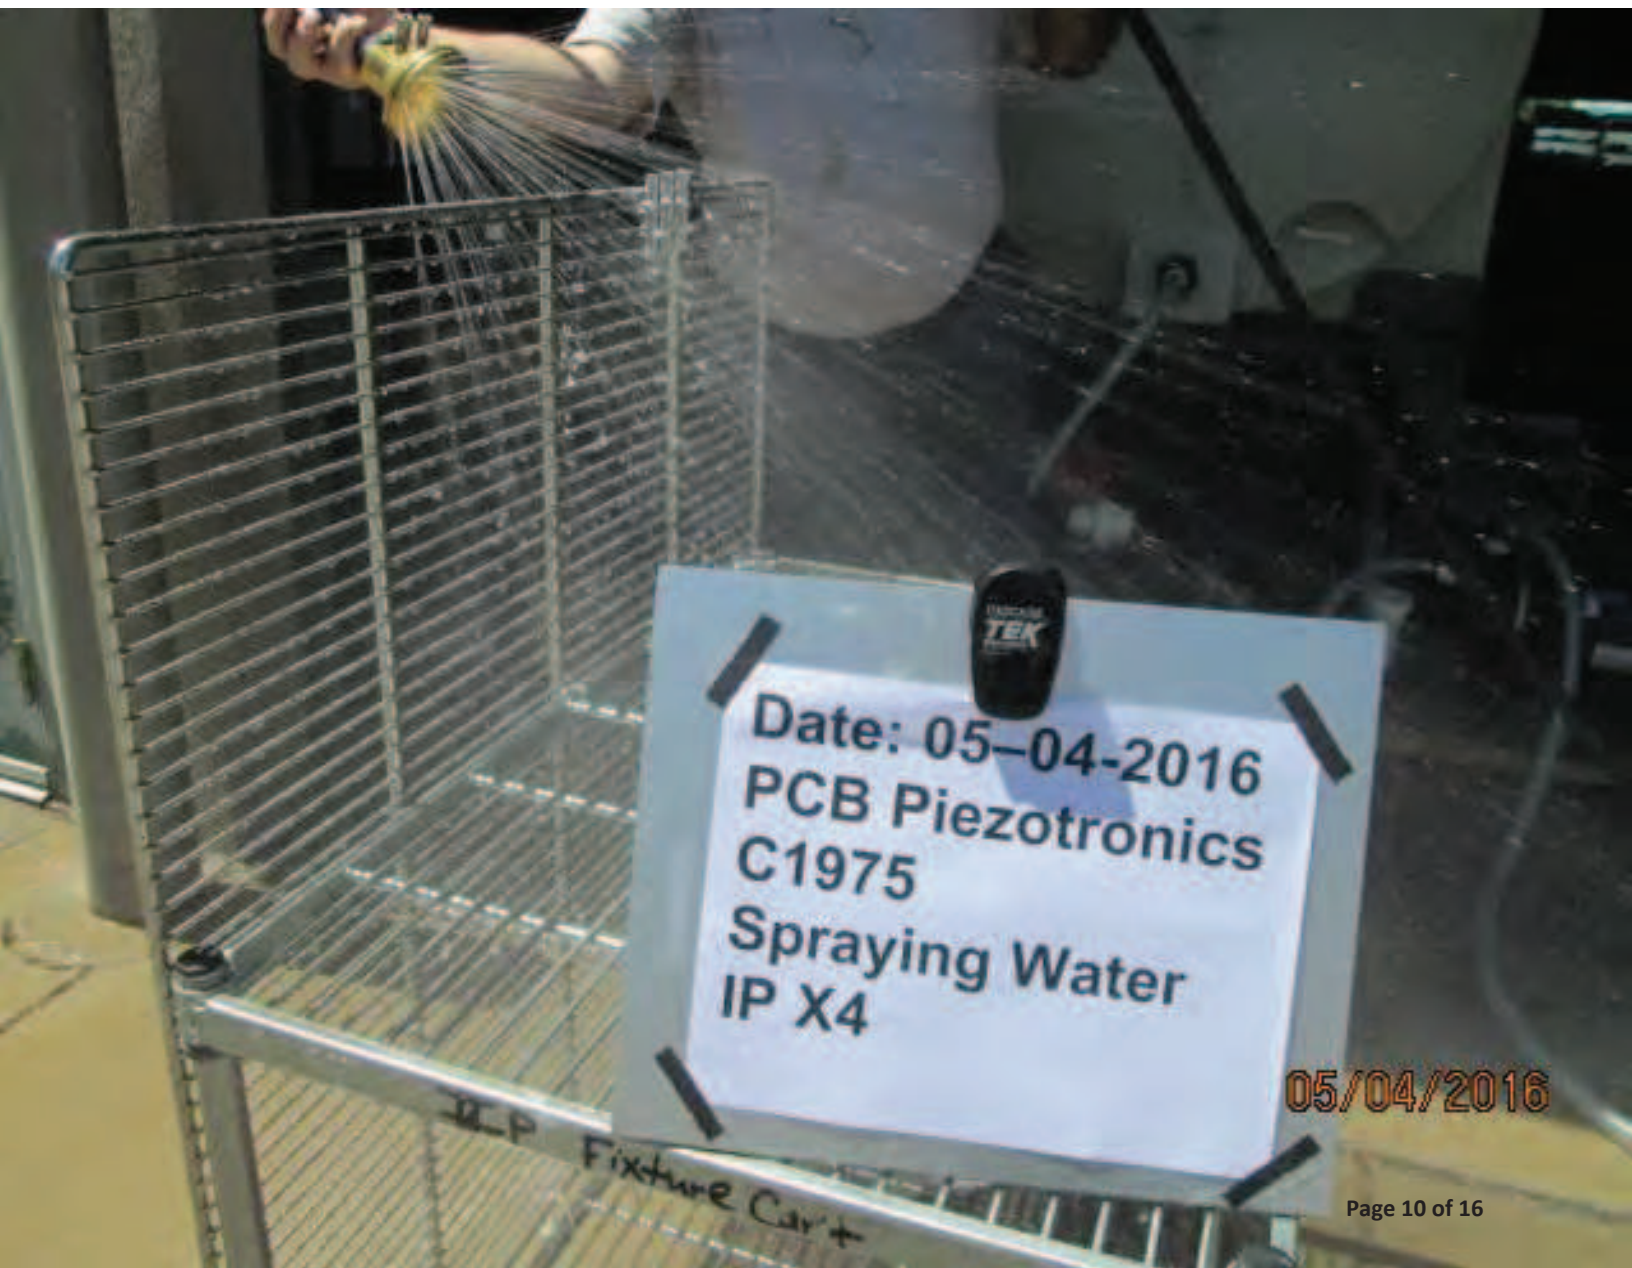

Date: 05-04-2016
PCB Piezotronics
C1975
Spraying Water
IP X4

05/04/2016

IP Fixture Cart

Date: 05-04-2016
PCB Piezotronics
C1975
Spraying Water
IP X4
Post Exposure

05/04/2016





Test Data Log – Protection Against Water (IPX1 through IPX9)

Section 1 – Customer and Test Information

Job Number: C1975

Customer: PCB Piezotronics

Date Started: 5/4/2016

Date Completed: 5/4/2016

QA Reviewer: Meg Talbert

Signature: *Meg Talbert*

Responsible Technician: Keefe Hart

Quote Issued By: Joe Fratiello

Customer Witness: No Yes Name: N/A

Section 2 – Test parameters

Type of Test: Protection Against Water Intrusion

Test Specification: IEC 60529, Ed. 2.2, Sec. 14.2.5

Test Description:

- IP Designation: IPX5
- Test Means: Spray nozzle $\pm 180^\circ$ from vertical.
- Water Flow Rate: 12.5 l/min $\pm 5\%$
- Water Temperature: The water temperature does not differ from that of the specimen by more than 5° K.
- Water Pressure: N/A
- Instructions on Disassembling the Specimen Have Been Received: Yes No
- Passing Criteria: In general, if any water has entered, it shall not:
 - Be sufficient to interfere with the correct operation of the equipment or impair safety.
 - Deposit on insulation parts where it could lead to tracking along the creepage distances.
 - Reach live parts or windings not designed to operate when wet.
 - Accumulate near the cable end or enter the cable if any.
- Additional Instructions: Water Jet Spray: Samples to be sprayed with a nozzle that has a 6.3mm diameter per Figure 6 from a distance of 2.5-3 meters. Water flow shall be at a rate of 12.5l/minute for a period of 1 minute per square meter of enclosure for a minimum of 3 minutes. Water temperature shall not differ by more than 5K from sample temperature. Water shall have no harmful effects on enclosure.
- Test Conditions: IEC 60529, Ed. 2.2, Sec. 14.2.5
- Test Duration: 1 min/m², minimum of 3 minutes.

Section 3 – Test Sample Information

Sample Description	Sample P/N or Model No.	Sample S/N or Other Identifier	Qty.
Microphones	130A24	44296	1
Microphones	130A24	44293	1
Microphones	130A24	44292	1

Section 4 – Test Equipment

ID No.	Description	Manufacturer	Model No.	Serial No.	Last Cal	Next Cal
FR84	Spray Nozzle	CTEK	6.3 MM	1	Factory Set	
FR506	Stop watch	Digi-Sense	94460-28	160157786	01/28/16	01/28/18
FR66	Tape Measure	Stanley	LeverLock	30-824	Verified Before Use	
FR135	Thermometer	Fluke	54 II B	20380005	06/17/15	06/17/16
FR512	Temperature/Relative Humidity Meter	Cole-Parmer	90080-03	160173042	03/05/16	03/05/18

Section 5 – Test Log

Customer Name: PCB Piezotronics
 Job Number: C1975

Laboratory Temperature: +71°F
 Laboratory Humidity: 26% RH

Initials	Date	Time	Notes	Photo
KH	5/4/2016	1250	Samples are mounted on a spray cart. Exposure will concentrate for the entire 3 minute exposure on the end of the microphone with the removable cover per customer direction.	<input checked="" type="checkbox"/>
KH	5/4/2016	1250	Water temperature is +16.5°C and sample temperature is +19.8°C; no thermal conditioning is necessary.	<input type="checkbox"/>
KH	5/4/2016	1250	Nozzle flow has been verified.	<input type="checkbox"/>
KH	5/4/2016	1251	Begin the 3 minute exposure.	<input checked="" type="checkbox"/>
KH	5/4/2016	1255	Exposure is complete.	<input type="checkbox"/>
KH	5/4/2016	1255	Samples are removed from the spray cart and hand dried.	<input type="checkbox"/>
KH	5/4/2016	1258	End covers are removed and exposed membrane is hand dried.	<input type="checkbox"/>
KH	5/4/2016	1300	Membrane pieces are removed and the interior of the sample is inspected for any indication of water presence.	<input checked="" type="checkbox"/>
KH	5/4/2016	1300	No water is detected inside of the samples.	<input checked="" type="checkbox"/>
KH	5/4/2016	1315	Samples will be returned to the customer for operational verification.	<input type="checkbox"/>
KH	5/4/2016	1315	Testing is complete.	<input type="checkbox"/>

CASCADE
TEK

Date: 05-04-2016
PCB Piezotronics
C1975
Water Jet Spray
IP X5

05/04/2016



Date: 05/04/2016
PCB Piezotronics
C1975
Water Jet Spray
IP X5

05/04/2016

Date: 05-04-2016

PCB Piezotronics

C1975

05/04/2016

Water Jet Spray

IP X5

Post Exposure





Cascade Technical Sciences, Inc.
Hillsboro, Oregon/Longmont Colorado

Report CTC C1975-2

May 31, 2016

For: PCB Piezotronics

Prepared By: **Meg Talbert** Digitally signed by Meg Talbert
DN: cn=Meg Talbert, o=Element Materials
Technology, ou=Quality,
email=meg.talbert@element.com, c=US
Date: 2016.05.31 20:41:50 -06'00'
 Element Denver Quality Administrator 05/31/2016
Date

Reviewed By: **Joe Fratiello** Digitally signed by Joe Fratiello
DN: cn=Joe Fratiello, o=Element Materials
Technology, ou=Laboratry,
email=Joe.Fratiello@Element.com, c=US
Date: 2016.06.01 10:52:53 -06'00'
 Element Denver Laboratory Manager 05/31/2016
Date

Concurred With: **Joe Fratiello** Digitally signed by Joe Fratiello
DN: cn=Joe Fratiello, o=Element
Materials Technology, ou=Laboratry,
email=Joe.Fratiello@Element.com, c=US
Date: 2016.06.01 10:53:29 -06'00'
 Element Portland Quality Manager 05/31/2016
Date
 (Denver Lab Manager signed in absence of QM)

EAR Controlled Data: This document contains technical data whose export and re-export/retransfer is subject to control by the U.S. Department of Commerce under the Export Administration Act and the Export Administration Regulations. The Department of Commerce's prior written approval may be required for the export or re-export/retransfer of such technical data to any foreign person, foreign entity or foreign organization whether in the United States or abroad.

These commodities, Technology, or software were exported from the United States in accordance with the Export Administration Regulations. Diversion contrary to U.S. law is prohibited.

It is our policy to retain components and sample remnants for a minimum of 30 days from the report date, after which time they may be discarded. The data herein represents only the item(s) tested. This report shall not be reproduced, except in full, without prior permission of Cascade Technical Sciences.

This project shall be governed exclusively by the General Terms and Conditions of Sale and Performance of Testing Services by Cascade Technical Sciences. In no event shall Cascade Technical Sciences be liable for any consequential, special or indirect loss or any damages above the cost of the work.

Administrative Data

Prepared for: PCB Piezotronics
3425 Walden Ave
Depew, NY 14043

Test Facility: Cascade Technical Sciences, Inc.
1530 Vista View Drive
Longmont, CO 80504

Test(s) Performed	Test Specification (Paragraph/Section)
Settling Dust	CEI/IEC 60529:2013 Para. 13.4 & 13.5

Item(s) Tested (Description)	Part Number(s)	Serial Number(s)
Microphones	130A24	44296
Microphones	130A24	44293
Microphones	130A24	44292

Rev.	Reason For Revision	Date	Approval
---	Report Issued.	05/19/2016	MJT
A	Corrected photos.	05/31/2016	MJT

Date Test Items Received: 03/01/2016

Testing Initiated Date: 03/15/2016

Testing Completed Date: 03/16/2016



Cascade Tek – Hillsboro, Oregon/Longmont, Colorado

May 31, 2016

Certification No: CTC C1975-2

Attention: Mr. Michael Thibeault
PCB Piezotronics
3425 Walden Ave
Depew, NY 14043

- Reference:
- a. CTek Job No.: C1975
 - b. CTek Quote No.: 18127A
 - c. Customer Purchase Order No.: WE00005021
 - d. Technical Specification: 1. CEI/IEC 60529: 2013

Cascade Technical Sciences, Inc. hereby certifies that the following test sample(s) were subjected to the following test(s).

Quantity	Description	Model/Part Number	Serial Number(s)
1	Microphones	130A24	44296
1	Microphones	130A24	44293
1	Microphones	130A24	44292

1. Dust Test per Reference (b) Item 3 and (d1), the non-operating samples were subjected to eight hours of dust exposure at a concentration of two kg/m³. No visible dust ingress was observed.

Testing was done in accordance with the above references as evidenced and reported in the accompanying data. The test samples were returned to the customer for evaluation.

The original of this report is on file at Cascade Technical Sciences, Inc. under the above referenced certification number for review by authorized personnel. The results of the testing reported herein relate only to the actual items tested.

Respectfully submitted,



Meg Talbert

Quality Administrator

Cascade Technical Sciences, Inc.

This test certification shall not be reproduced, except in full, without written authorization from Cascade Technical Sciences, Inc.

The objective of this test program was to subject customer provided test hardware to environmental simulation in compliance with customer stated specification, including any authorized modification, deviations or concessions to the original requirements. The hardware consisted of items identified in the appropriate sections of this report. In addition to test hardware identification, each section contains information that describes the associated test setup and performance and the resulting data. Cascade Technical Sciences, Inc. measuring instruments used in testing were calibrated according to the requirements of ANSI/NCSL Z540-1 and ISO/IEC 17025, and are traceable NIST or NMI. Calibration records are on file and available for inspection by request. Because the test methods are well established and are qualitative or semi-quantitative in nature, Cascade Technical Sciences, Inc., Inc. does not apply measurement uncertainty unless obligated by contract. Any test hardware operational setups and resulting evaluations or inspections performed by the customer are not included in this report, unless they were explicitly requested. While observations and/or specification compliance statements may be reported, no interpretations or opinions regarding customer product performance are intended. Unless otherwise indicated in the appropriate report section, all contract obligations were met and the test objective achieved.



Test Data Log – Protection Against Solid Foreign Objects (IP5X through IP6X)

Section 1 – Job Information

Job Number: C1975

Customer: PCB Piezotronics

Date Started: 3/15/2016

Date Completed: 3/16/2016

QA Reviewer: Meg Talbert

Signature: *Meg Talbert*

Responsible Technician: Keefe Hart

Quote Issued By: Joe Fratiello

Customer Witness: No Yes Name: N/A

Section 2 – Test Parameters

Type of Test: Settling Dust

Test Specification: IEC 60529: 2013 Ed. 2.2, Sec. 13.4 & 13.5

Test Description:

- IP Designation: IP5X
- Enclosure Category: 2 - No pressure difference.
- Dust: 2 kg of talcum powder per cubic meter of the test chamber volume.
- Air On: 2 seconds
- Air Off: 3 minutes
- Number of Cycles: 160
- Total Test Time: 8 hours
- Instructions on Disassembling the Specimen Have Been Received: Yes No
- Passing Criteria: No deposit of dust is observable inside the enclosure at the end of the test.
- Additional Instructions:

Section 3 – Test Sample Information

Sample Description	Sample P/N or Model No.	Sample S/N or Other Identifier	Qty.
Microphones	130A24	44296	1
Microphones	130A24	44293	1
Microphones	130A24	44292	1

Section 4 – Test Equipment

ID No.	Description	Manufacturer	Model No.	Serial No.	Last Cal	Next Cal
1224	Dust Chamber	Thermotron	D27	29644	Reference Only	
FR71	Test Dust	Equate	Talcum Powder	NA	Factory Mix	
FR449	Dust Sieve	Dual Manufacturing	SP8-2	200	Reference Only	
FR72	Manometer	Dwyer	24-D	3343	Reference Only	
FR422	Electronic Precision Balance	Mettler Toledo	PR5002	1120271907	01/28/16	01/28/17
FR494	Stop Watch	Control Company	94460-28	140586526	01/29/15	01/29/17
FR513	Temperature/Relative Humidity Meter	Cole-Parmer	90080-03	160173038	03/05/16	03/05/18

Section 5 – Test Log

Customer Name: PCB Piezotronics

Laboratory Temperature: +70°F

Job Number: C1975

Laboratory Humidity: 20% RH

Initials	Date	Time	Notes	Photo
KH	3/15/2016	1500	Samples are placed in dust chamber.	<input checked="" type="checkbox"/>
KH	3/15/2016	1515	Begin 8 hour exposure.	<input type="checkbox"/>
KH	3/16/2016	0800	8 hour exposure is complete.	<input type="checkbox"/>
KH	3/16/2016	0815	Brush excess dust off of the exterior of the samples	<input type="checkbox"/>
KH	3/16/2016	0815	Remove samples from dust chamber and hand clean the exterior of the sample to remove any remaining dust.	<input type="checkbox"/>
KH	3/16/2016	0820	All 3 samples have visible dust collection inside of the connector end.	<input checked="" type="checkbox"/>
KH	3/16/2016	0820	The end cap and black cover are removed from all 3 samples. No dust ingress under the black cover is observed.	<input checked="" type="checkbox"/>
KH	3/16/2016	0830	Samples will remain on site for further testing.	<input type="checkbox"/>
KH	3/16/2016	0830	Dust testing is complete.	<input type="checkbox"/>

Date: 03-16-16
PCB Piezotronics
Job# C1975
Dust
IP 5X
Post Exposure

03/16/2016



03/16/2016



03/16/2016

Date: 03 - 16 - 16

PCB Piezotronics

Job# C1975

Dust

IP-5X

Post Exposure



03/16/2016

Job# C1975

Dust

IP-5X

Post Exposure



03/16/2016